



Test Report: MSP-1000-48

1000W Single Output Medical Type

■ DESIGN VERIFY TEST

Output Function Test

Input Function Test

Protection Function Test

Control Function Test

Component Stress Test

■ SAFETY & E.M.C. TEST

Safety Test

E.M.C. Test

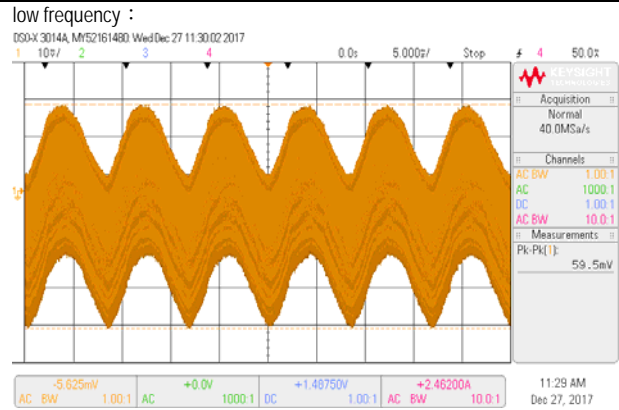
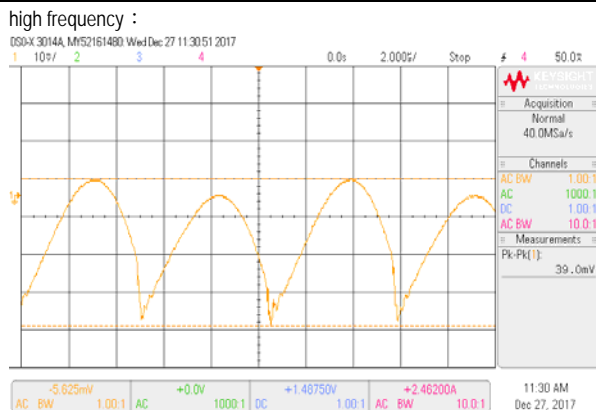
■ RELIABILITY TEST

ENVIRONMENT TEST



DESIGN VERIFY TEST







OUTPUT FUNCTION TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	OUTPUT VOLTAGE ADJUST RANGE	CH1: 46V~ 56 V	I/P : 230 VAC I/P : 115 VAC O/P : MIN LOAD Ta : 25°C	43.57V~57.76V/230VAC 43.68V~57.73V/115VAC
2	OUTPUT VOLTAGE(Max) TOLERANCE	V1: 1%~ -1%	I/P: 200VAC /264VAC O/P:FULL/ MIN. LOAD Ta:25°C	V1: 0.31%~ 0%
3	LINE REGULATION (Max)	V1: 0.5%~ -0.5 %	I/P: 200VAC~ 264VAC O/P:FULL LOAD Ta:25°C	V1: 0 %
4	LOAD REGULATION(Max)	V1: 0.5%~ -0.5 %	I/P: 230VAC O/P:FULL ~MIN LOAD Ta:25°C	V1: 0 %
5	OVER/UNDERSHOOT TEST	< ±5%	I/P: 230VAC O/P:FULL LOAD Ta:25°C	< 5 %
6	RIPPLE & NOISE(Max)	V1: 250mVp-p	I/P:230VAC O/P:FULL LOAD Ta:25°C	V1: 39 mVp-p




7	SET UP TIME(Max)	230VAC/1000ms 115VAC/2000ms	I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C	230VAC/ 437 ms 115VAC/ 411 ms
---	------------------	--------------------------------	--	----------------------------------

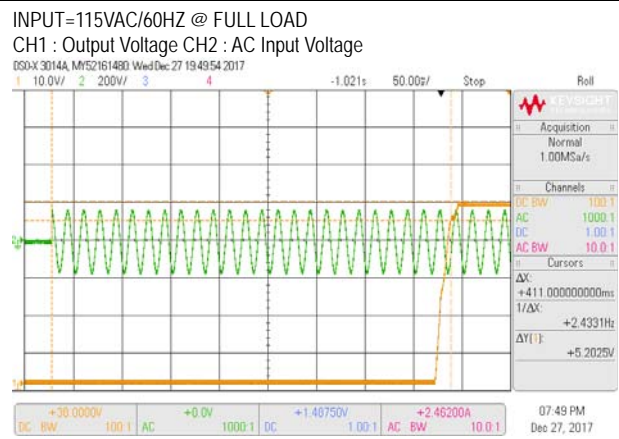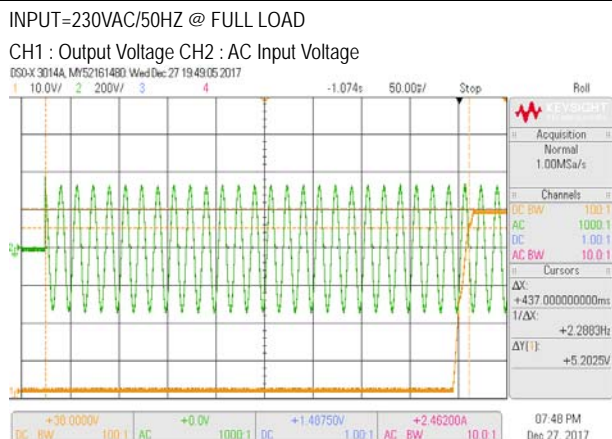

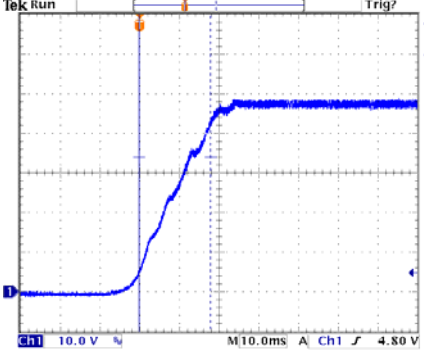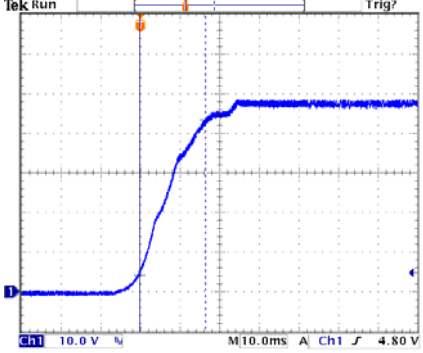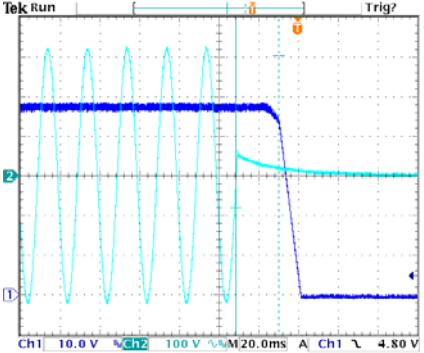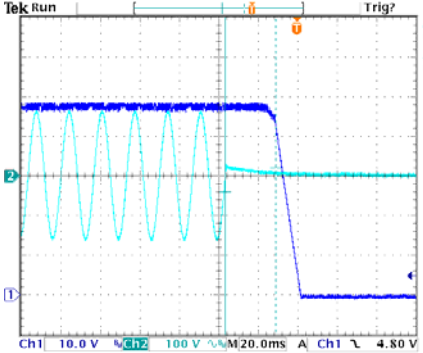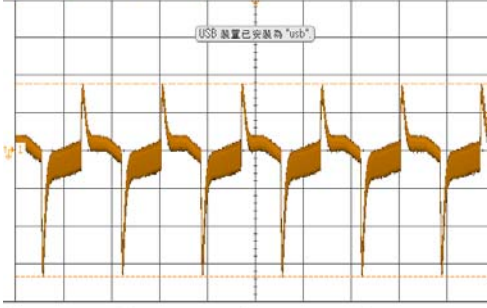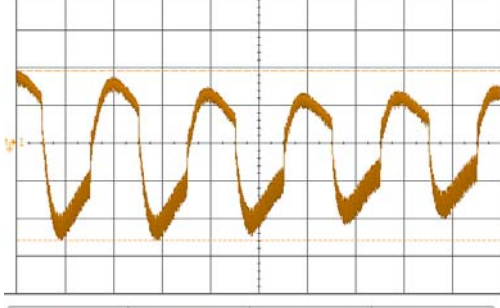
8 RISE TIME (Max)	230VAC/50ms 115VAC/50ms	I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C	230VAC/18 ms 115VAC/ 16.6 ms
INPUT=230VAC/50HZ @ FULL LOAD CH1 : Output Voltage 		INPUT=115VAC/60HZ @ FULL LOAD CH1 : Output Voltage 	
9 HOLD UP TIME (Typ.)	230VAC/16ms 115VAC/16ms	I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C	230VAC/21.6 ms 115VAC/25.6 ms
INPUT=230VAC/50HZ @ FULL LOAD CH1 : Output Voltage CH2 : AC Input Voltage 		INPUT=115VAC/60HZ @ FULL LOAD CH1 : Output Voltage CH2 : AC Input Voltage 	
10 DYNAMIC LOAD	V1: 4800 mVp-p	I/P: 230VAC O/P: (1)FULL /50% LOAD 50%DUTY / 120HZ (2)FULL /50% LOAD 50%DUTY / 1KHZ Ta:25°C	255mVp-p 225mVp-p
FULL /50% LOAD 50%DUTY / 120HZ 		FULL /50% LOAD 50%DUTY / 1KHZ 	

INPUT FUNCTION TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT																																	
1	INPUT VOLTAGE RANGE	90VAC~264VAC	I/P:TESTING O/P:FULL LOAD Ta:25°C	73V~264V																																	
			I/P: LOW-LINE-3V=87 V HIGH-LINE+15%=300 V O/P:FULL/MIN LOAD (PLEASE CHECK DERATING CURVE) ON: 30 Sec OFF: 30 Sec 10MIN (POWER ON/OFF NO DAMAGE)	TEST:OK																																	
2	INPUT FREQUENCY RANGE	47HZ ~63 HZ NO DAMAGE	I/P:100 VAC ~264 VAC O/P:FULL-MIN LOAD Ta:25°C	TEST: OK																																	
3	INPUT CURRENT (Typ.)	230V/ 5A 115V/ 8.5A	I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C	I=4.8A/ 230VAC I=8.21A/ 115VAC																																	
4	LEAKAGE CURRENT	Earth leakage current < 360 uA/264VAC	I/P : 264 VAC O/P : Min LOAD Ta : 25°C	L-FG : 300uA N-FG : 298uA																																	
		Touch leakage current < 100 uA/264VAC	I/P : 264 VAC O/P : Min LOAD Ta : 25°C	L-V+ : 84.6uA L-V-: 84.7uA N-V+: 84.5uA N-V-: 84.6uA																																	
5	NO LOAD CONSUMPTION	< 0.75W	I/P : 115VAC I/P : 230VAC O/P : NO LOAD Ta : 25°C	< 0.412 W < 0.671 W																																	
6	POWER FACTOR (Typ.)	0.95/ 230VAC 0.98/115VAC	I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C	PF=0.973/230VAC PF=0.996/115VAC																																	
<p>P.F vs LOAD</p> <table border="1"> <caption>Approximate data from P.F vs LOAD graph</caption> <thead> <tr> <th>LOAD (%)</th> <th>PF (115VAC)</th> <th>PF (230VAC)</th> </tr> </thead> <tbody> <tr><td>10%</td><td>0.90</td><td>0.65</td></tr> <tr><td>20%</td><td>0.95</td><td>0.82</td></tr> <tr><td>30%</td><td>0.97</td><td>0.88</td></tr> <tr><td>40%</td><td>0.98</td><td>0.92</td></tr> <tr><td>50%</td><td>0.99</td><td>0.94</td></tr> <tr><td>60%</td><td>0.99</td><td>0.95</td></tr> <tr><td>70%</td><td>0.99</td><td>0.96</td></tr> <tr><td>80%</td><td>0.99</td><td>0.97</td></tr> <tr><td>90%</td><td>0.99</td><td>0.97</td></tr> <tr><td>100%</td><td>0.99</td><td>0.98</td></tr> </tbody> </table>					LOAD (%)	PF (115VAC)	PF (230VAC)	10%	0.90	0.65	20%	0.95	0.82	30%	0.97	0.88	40%	0.98	0.92	50%	0.99	0.94	60%	0.99	0.95	70%	0.99	0.96	80%	0.99	0.97	90%	0.99	0.97	100%	0.99	0.98
LOAD (%)	PF (115VAC)	PF (230VAC)																																			
10%	0.90	0.65																																			
20%	0.95	0.82																																			
30%	0.97	0.88																																			
40%	0.98	0.92																																			
50%	0.99	0.94																																			
60%	0.99	0.95																																			
70%	0.99	0.96																																			
80%	0.99	0.97																																			
90%	0.99	0.97																																			
100%	0.99	0.98																																			
7	EFFICIENCY(Typ.)	94%	I/P:230 VAC O/P:FULL LOAD Ta:25°C	94.2 %																																	

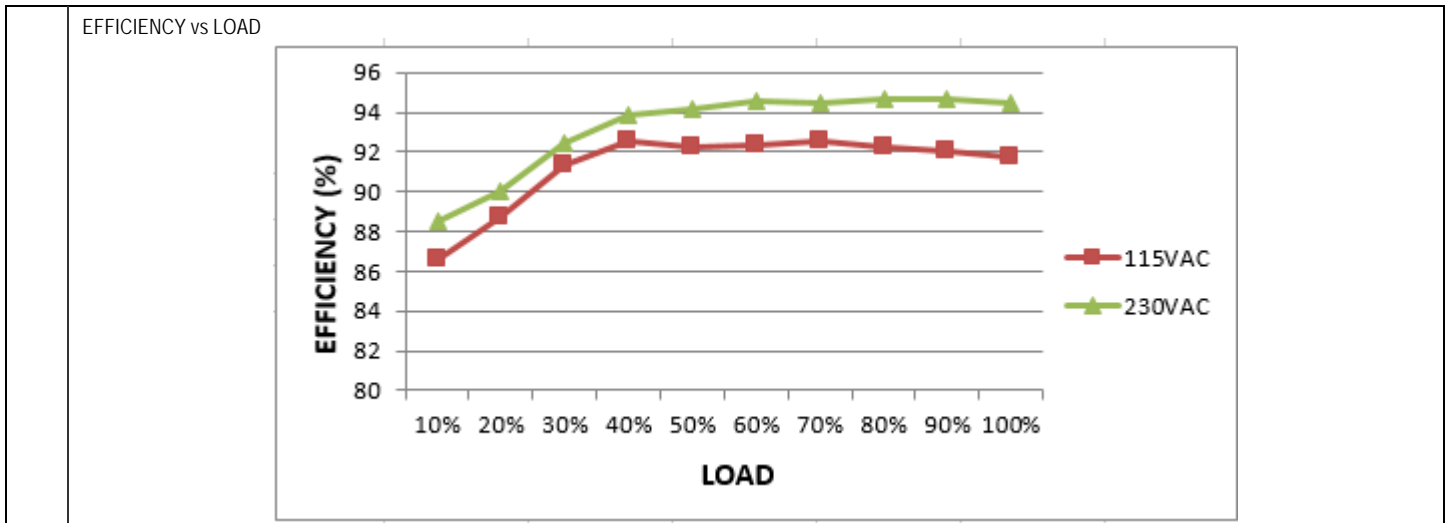

8	INRUSH CURRENT(Typ.)	230V/40A 115V/20A COLD START	I/P : 230 VAC I/P : 115 VAC O/P : FULL LOAD Ta : 25°C	I =30.5A/ 230VAC I =17A/ 115VAC T50= 1380 us/230V
---	----------------------	------------------------------------	--	---

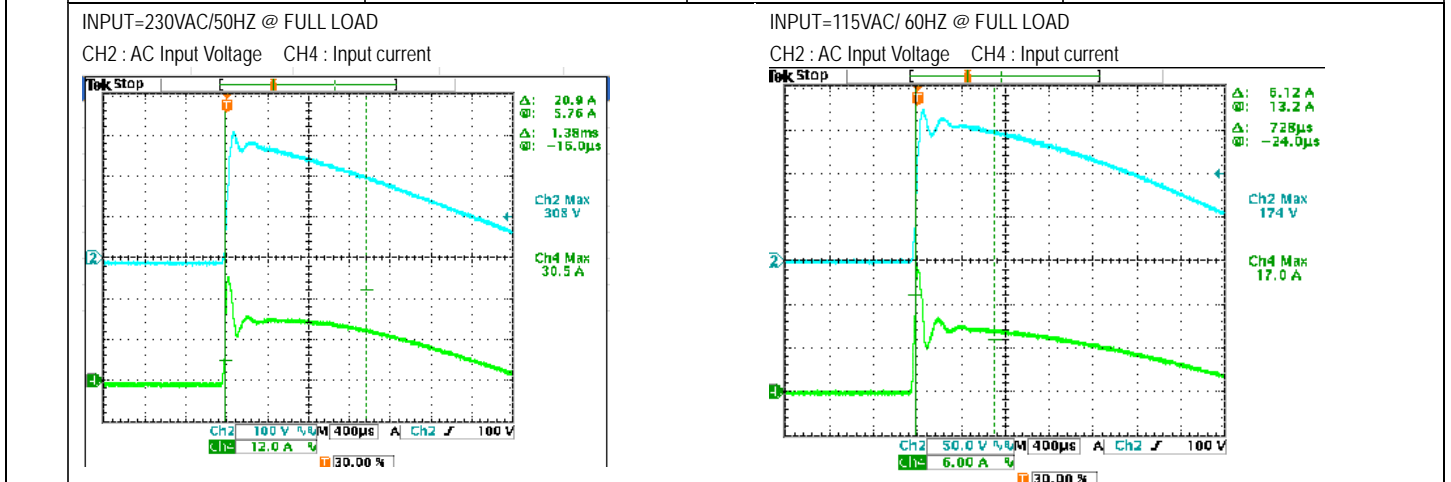



PROTECTION FUNCTION TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	OVER LOAD PROTECTION	105%~ 135 % Protection type : Constant current limiting, recovers automatically after fault condition is removed	I/P: 264VAC I/P: 230VAC I/P: 200AC O/P: TESTING Ta:25°C	115.03%/ 264VAC 115.03%/ 230VAC 115.04%/200VAC PROTECTION TYPE : Constant current limiting, recovers automatically after fault condition is removed

2	OVER VOLTAGE PROTECTION	58V-65V Protection type : Shut down o/p voltage, re-power on to recover	I/P: 264VAC I/P: 230VAC I/P: 90VAC O/P: MIN LOAD Ta:25°C	60.97V/ 264VAC 60.97V/ 230VAC 60.98V/ 90VAC PROTECTION TYPE : Shut down o/p voltage, re-power on to recover
3	OVER TEMPERATURE PROTECTION	Protection type : Shut down o/p voltage, recovers automatically after temperature goes down	I/P: 264VAC I/P: 90VAC O/P: FULL LOAD	O.T.P. Active Protection type : Shut down o/p voltage, recovers automatically after temperature goes down
4	SHORT PROTECTION	SHORT EVERY OUTPUT 1 HOUR NO DAMAGE PROTECTION TYPE :	I/P: 264VAC I/P: 90VAC O/P: FULL LOAD Ta:25°C	NO DAMAGE PROTECTION TYPE : Constant current limiting, recovers automatically after fault condition is removed

CONTROL FUNCTION TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT						
1	CURRENT SHARING	< 10%	I/P : 230 VAC O/P : FULL/50% LOAD Ta : 25°C	O/P : 90% PSU1 : 19.4A PSU2 : 19.3A PSU3 : 19.4A PSU4 : 20.3A O/P : 50% PSU1 : 10.9A PSU2 : 10.2A PSU3 : 10.3A PSU4 : 11.8A						
2	REMOTE ON/OFF CONTROL	<p>The PSU can be turned ON/OFF by using the "Remote Control" function.</p> <table border="1"> <tr> <td>Between RC+(pin3) and RC-(pin4)</td> <td>Output Status</td> </tr> <tr> <td>SW ON (Short)</td> <td>ON</td> </tr> <tr> <td>SW OFF (Open)</td> <td>OFF</td> </tr> </table> <p>I/P: 230 VAC O/P: FULL LOAD Ta:25°C TEST RESULT : OK</p>	Between RC+(pin3) and RC-(pin4)	Output Status	SW ON (Short)	ON	SW OFF (Open)	OFF		
Between RC+(pin3) and RC-(pin4)	Output Status									
SW ON (Short)	ON									
SW OFF (Open)	OFF									
3	REMOTE SENSE	S+ / S- >0.5V								

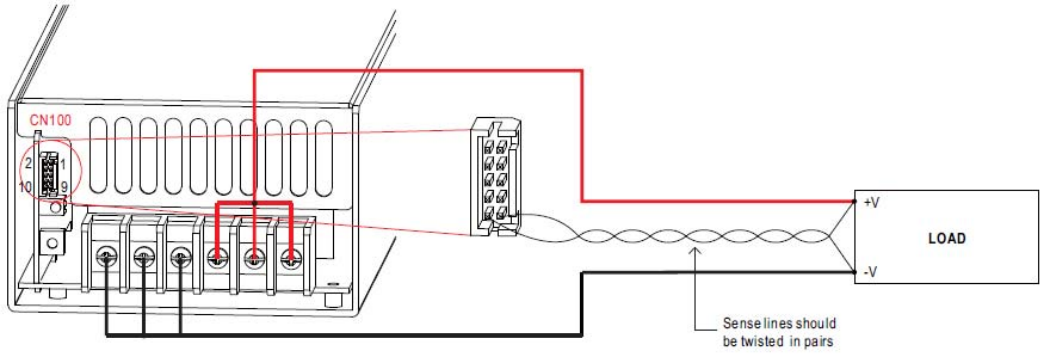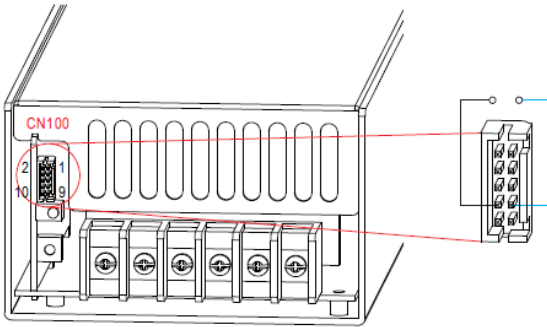		 <p>I/P: 230 VAC O/P: FULL LOAD Ta: 25°C TEST RESULT: > 0.5 V</p>											
4	DC OK SIGNAL	<p>The TTL signal out, PSU turn on = 3.3 ~ 5.6V ; PSU turn off = 0 ~ 1V DC-OK signal is a TTL level signal. High when PSU turns on.</p> <table border="1" data-bbox="459 929 817 1032"> <thead> <tr> <th>Between DC-OK(pin7) and GND(pin6,8)</th> <th>Output Status</th> </tr> </thead> <tbody> <tr> <td>3.3 ~ 5.6V</td> <td>ON</td> </tr> <tr> <td>0 ~ 1V</td> <td>OFF</td> </tr> </tbody> </table>  <p>I/P: 230VAC O/P: FULL LOAD Ta: 25°C TEST RESULT: PSU turn on = 5.27V PSU turn off = 0.005V</p>	Between DC-OK(pin7) and GND(pin6,8)	Output Status	3.3 ~ 5.6V	ON	0 ~ 1V	OFF					
Between DC-OK(pin7) and GND(pin6,8)	Output Status												
3.3 ~ 5.6V	ON												
0 ~ 1V	OFF												
5	5V STANDBY	5VSB : 5V@0.3A ; tolerance ± 5%, ripple : 50mVp-p(max.)	I/P: 230 VAC O/P: FULL LOAD Ta: 25°C	TEST RESULT : 5.035V /0.3A Ripple : 3.2 mVp-p									
6	FAN CONTROL	FAN ON/OFF BY BY NTC (RT50) OR LOAD	I/P: 230 VAC O/P: TESTING	<table border="1" data-bbox="1150 1608 1501 1709"> <thead> <tr> <th></th> <th>TEMP.</th> <th>LOAD</th> </tr> </thead> <tbody> <tr> <td>FAN ON</td> <td>55°C</td> <td>>10.4%</td> </tr> <tr> <td>FAN OFF</td> <td>36°C</td> <td><10%</td> </tr> </tbody> </table>		TEMP.	LOAD	FAN ON	55°C	>10.4%	FAN OFF	36°C	<10%
	TEMP.	LOAD											
FAN ON	55°C	>10.4%											
FAN OFF	36°C	<10%											

COMPONENT STRESS TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	PWM Transistor (D to S) or (C to E) Peak Voltage	Q911 Rated: 26A / 600V	I/P: High-Line +3V = 303V AC ON/OFF VDS: O/P: (1) Full Load (2) Output Short	VDS: (1) 506V (2) 490V

			(3)Dynamic Load Full Load/ Min. Load 90%Duty/1KHz (4)Dynamic Load Full Load/ Min. Load 90%Duty/3KHz (5)Dynamic Load Full Load/ Min. Load 90%Duty/5KHz (6)Dynamic Load 100% Load/ Min. Load 50%Duty/120Hz (7)0%→400% Load. Ta:25°C	(3)510V (4)510V (5)506V (6)510V (7)490V
2	P.F.C Transistor (D to S) or (C to E) Peak Voltage	Q1 Rated: 34A / 600V	I/P:High-Line +3V =303V V AC ON/OFF O/P: (1)Full Load (2)Output Short (3)Dynamic Load Full Load/ Min. Load 90%Duty/1KHz (4)Dynamic Load Full Load/ Min. Load 90%Duty/3KHz (5)Dynamic Load Full Load/ Min. Load 90%Duty/5KHz (6)Dynamic Load 100% Load/ Min. Load 50%Duty/120Hz (7)0%→400% Load. Ta:25°C	VDS: (1) 490V (2) 510V (3) 502V (4) 506V (5) 510V (6) 506V (7) 494V
3	P.F.C DIODE	D6 Rated: 10A / 600V	I/P:High-Line +3V =303V V AC ON/OFF O/P: (1)Full Load (2)Output Short (3)Dynamic Load Full Load/ Min. Load 90%Duty/5KHz (4)Dynamic Load 100% Load/ Min. Load 50%Duty/120Hz Ta:25°C	(1) 405V (2) 413V (3) 389V (4) 397V
4	SR MOSFET Peak Voltage	Q508 Rated: 76A / 150V Q506 Rated: 76A / 150V	I/P:High-Line +3V =303V V AC ON/OFF O/P: (1)Full Load (2)Output Short (3)Dynamic Load Full Load/ Min. Load 90%Duty/1KHz (4)Dynamic Load Full Load/ Min. Load 90%Duty/3KHz (5)Dynamic Load Full Load/ Min. Load 90%Duty/5KHz (6)Dynamic Load 100% Load/ Min. Load 50%Duty/120Hz (7)0%→400% Load. (8).NO LOAD (9) burst mode Ta:25°C	Q508: Q506: VDS: VDS: (1)118.2V (1)119.4V (2)6.0V (2)13.3V (3)118.6V (3)118.6V (4)117.8V (4)120.2V (5)116.2V (5)118.6V (6)117.8V (6)118.6V (7)113.8V (7)114.6V (8)48.4V (8)113.8V (9)116.2V (9)117.8V
5	Input Capacitor Voltage	C5 220μF / 400V	I/P:High-Line +3V =303VV O/P: (1)Full Load input on/off (2) Min load input on /Off (3)Full Load /Min load Change (4)Full load continue Ta:25°C	(1)399V (2)399V (3)398V (4) 398V

6	Control IC Voltage Test	<p>PFC IC U1 Absolute Rating: -0.3 V ~ 26 V Operating Range: 12.9 V ~ 25 V</p> <p>PWM IC U900 Absolute Rating: Self-limited Operating Range: 8.85 V ~ 16 V</p>	<p>I/P:High-Line +3V =303V V AC ON/OFF O/P(1)FULL LOAD (2) Output Short (3)O.L.P (4)O.V.P. (5)NO LOAD VRmin .LOW LINE Ta:25°C</p>	<p>(1) 21.5V (2) 21.9V (3) 21.3V (4) 19.5V (5) 15.2V</p> <p>(1) 14.63V (2) 14.87V (3) 15.03V (4) 14.07V (5) 13.51V</p>
7	TOP SWITCHING STAND BY POWER	U971 Rated : 1.8 A / 700V	<p>I/P:High-Line +3V =303V V AC ON/OFF O/P: (1)Full Load (2)Remote On/Off Ta:25°C</p>	<p>(1) 535V (2) 543V</p>

SAFETY TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	WITHSTAND VOLTAGE	<p>I/P-O/P: 4.5KVAC/min I/P-FG :2KVAC/min O/P-FG:1.5KVAC/min</p>	<p>I/P-O/P: 4.6 KVAC/min I/P-FG: 2.4 KVAC/min O/P-FG:1.8KVAC/min Ta:25°C</p>	<p>I/P-O/P:6.7mA I/P-FG:5.44mA O/P-FG:5.2mA NO DAMAGE</p>
2	ISOLATION RESISTANCE	<p>I/P-O/P:500VDC>100MΩ I/P-FG: 500VDC>100MΩ O/P-FG:500VDC>100MΩ</p>	<p>I/P-O/P: 500 VDC I/P-FG: 500 VDC O/P-FG: 500 VDC Ta:25°C</p>	<p>I/P-O/P: 23.8GΩ I/P-FG:23.2 GΩ O/P-FG:30 GΩ NO DAMAGE</p>
3	GROUNDING CONTINUITY	<p>FG(PE) TO CHASSIS OR TRACE < 100 mΩ</p>	<p>40A / 2min Ta:25°C</p>	<p>13 mΩ</p>

E.M.C TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	HARMONIC	<p>EN61000-3-2 CLASS A</p>	<p>I/P:230VAC/50HZ O/P:FULL LOAD Ta:25°C</p>	<p>PASS</p>
2	CONDUCTION	<p>EN55032 /EN55011 CLASS B</p>	<p>I/P : 230 VAC (50HZ) O/P : FULL/50% LOAD Ta : 25°C</p>	<p>PASS Test by certified Lab</p>
3	RADIATION	<p>EN55032 /EN55011 CLASS B</p>	<p>I/P : 230 VAC (50HZ) O/P : FULL LOAD Ta : 25°C</p>	<p>PASS Test by certified Lab</p>
4	E.S.D	<p>EN61000-4-2 MEDICAL AIR: 15KV / Contact: 8KV</p>	<p>I/P : 230 VAC/50HZ O/P : FULL LOAD Ta : 25°C</p>	<p>CRITERIA A</p>
5	E.F.T	<p>EN61000-4-4 MEDICAL INDUSTRY INPUT : 2KV</p>	<p>I/P : 230 VAC/50HZ O/P : FULL LOAD Ta : 25°C</p>	<p>CRITERIA A</p>
6	SURGE	<p>IEC61000-4-5 MEDICAL INDUSTRY L-N : 2KV L,N-PE : 4KV</p>	<p>I/P : 230 VAC/50HZ O/P : FULL LOAD Ta : 25°C</p>	<p>CRITERIA A</p>

7	Test by certified Lab & Test Report Prepare
---	---

■ **RELIABILITY TEST**

ENVIRONMENT TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT																																																																																																																																																				
1	TEMPERATURE RISE TEST	MODEL : MSP-1000-48 1. ROOM AMBIENT BURN-IN : 1.5 HRS I/P : 230VAC O/P : FULL LOAD Ta= 25 °C 2. HIGH AMBIENT BURN-IN : 1 HRS I/P : 230VAC O/P : FULL LOAD Ta= 60 °C																																																																																																																																																						
				<table border="1"> <thead> <tr> <th>NO</th> <th>Position</th> <th>ROOM AMBIENT Ta= 25 °C</th> <th>HIGH AMBIENT Ta= 60 °C</th> </tr> </thead> <tbody> <tr><td>1</td><td>BD1</td><td>47.0°C</td><td>83.0°C</td></tr> <tr><td>2</td><td>R6</td><td>48.5°C</td><td>85.1°C</td></tr> <tr><td>3</td><td>Q1</td><td>40.5°C</td><td>77.3°C</td></tr> <tr><td>4</td><td>U1</td><td>39.9°C</td><td>76.1°C</td></tr> <tr><td>5</td><td>D5</td><td>35.5°C</td><td>71.9°C</td></tr> <tr><td>6</td><td>D6</td><td>45.3°C</td><td>83.1°C</td></tr> <tr><td>7</td><td>C6</td><td>33.0°C</td><td>68.5°C</td></tr> <tr><td>8</td><td>D981</td><td>40.0°C</td><td>76.3°C</td></tr> <tr><td>9</td><td>RY1</td><td>36.3°C</td><td>73.0°C</td></tr> <tr><td>10</td><td>RG2</td><td>45.3°C</td><td>82.2°C</td></tr> <tr><td>11</td><td>D431</td><td>46.3°C</td><td>81.4°C</td></tr> <tr><td>12</td><td>C406</td><td>26.6°C</td><td>62.7°C</td></tr> <tr><td>13</td><td>TSW4</td><td>34.2°C</td><td>70.6°C</td></tr> <tr><td>14</td><td>L1</td><td>47.5°C</td><td>82.2°C</td></tr> <tr><td>15</td><td>T951</td><td>39.7°C</td><td>75.8°C</td></tr> <tr><td>16</td><td>C2</td><td>33.0°C</td><td>69.6°C</td></tr> <tr><td>17</td><td>LF3</td><td>36.5°C</td><td>73.5°C</td></tr> <tr><td>18</td><td>T1-1</td><td>51.5°C</td><td>87.4°C</td></tr> <tr><td>19</td><td>T1-2</td><td>48.4°C</td><td>84.4°C</td></tr> <tr><td>20</td><td>T2-1</td><td>49.9°C</td><td>85.6°C</td></tr> <tr><td>21</td><td>T2-2</td><td>42.7°C</td><td>79.1°C</td></tr> <tr><td>22</td><td>L900</td><td>43.3°C</td><td>80.2°C</td></tr> <tr><td>23</td><td>Q910</td><td>50.1°C</td><td>90.1°C</td></tr> <tr><td>24</td><td>C933</td><td>31.2°C</td><td>67.4°C</td></tr> <tr><td>25</td><td>Q911</td><td>47.4°C</td><td>87.0°C</td></tr> <tr><td>26</td><td>U900</td><td>30.4°C</td><td>66.6°C</td></tr> <tr><td>27</td><td>C906</td><td>26.7°C</td><td>62.9°C</td></tr> <tr><td>28</td><td>C106</td><td>30.9°C</td><td>67.2°C</td></tr> <tr><td>29</td><td>C109</td><td>28.0°C</td><td>64.0°C</td></tr> <tr><td>30</td><td>U501</td><td>33.0°C</td><td>69.7°C</td></tr> <tr><td>31</td><td>Q502</td><td>44.3°C</td><td>81.2°C</td></tr> <tr><td>32</td><td>Q504</td><td>43.1°C</td><td>79.6°C</td></tr> <tr><td>33</td><td>U504</td><td>37.2°C</td><td>73.8°C</td></tr> <tr><td>34</td><td>Q506</td><td>51.5°C</td><td>88.7°C</td></tr> <tr><td>35</td><td>Q508</td><td>43.4°C</td><td>80.3°C</td></tr> <tr><td>36</td><td>TSW3</td><td>27.6°C</td><td>63.7°C</td></tr> </tbody> </table>	NO	Position	ROOM AMBIENT Ta= 25 °C	HIGH AMBIENT Ta= 60 °C	1	BD1	47.0°C	83.0°C	2	R6	48.5°C	85.1°C	3	Q1	40.5°C	77.3°C	4	U1	39.9°C	76.1°C	5	D5	35.5°C	71.9°C	6	D6	45.3°C	83.1°C	7	C6	33.0°C	68.5°C	8	D981	40.0°C	76.3°C	9	RY1	36.3°C	73.0°C	10	RG2	45.3°C	82.2°C	11	D431	46.3°C	81.4°C	12	C406	26.6°C	62.7°C	13	TSW4	34.2°C	70.6°C	14	L1	47.5°C	82.2°C	15	T951	39.7°C	75.8°C	16	C2	33.0°C	69.6°C	17	LF3	36.5°C	73.5°C	18	T1-1	51.5°C	87.4°C	19	T1-2	48.4°C	84.4°C	20	T2-1	49.9°C	85.6°C	21	T2-2	42.7°C	79.1°C	22	L900	43.3°C	80.2°C	23	Q910	50.1°C	90.1°C	24	C933	31.2°C	67.4°C	25	Q911	47.4°C	87.0°C	26	U900	30.4°C	66.6°C	27	C906	26.7°C	62.9°C	28	C106	30.9°C	67.2°C	29	C109	28.0°C	64.0°C	30	U501	33.0°C	69.7°C	31	Q502	44.3°C	81.2°C	32	Q504	43.1°C	79.6°C	33	U504	37.2°C	73.8°C	34	Q506	51.5°C	88.7°C	35	Q508	43.4°C	80.3°C	36	TSW3	27.6°C	63.7°C
NO	Position	ROOM AMBIENT Ta= 25 °C	HIGH AMBIENT Ta= 60 °C																																																																																																																																																					
1	BD1	47.0°C	83.0°C																																																																																																																																																					
2	R6	48.5°C	85.1°C																																																																																																																																																					
3	Q1	40.5°C	77.3°C																																																																																																																																																					
4	U1	39.9°C	76.1°C																																																																																																																																																					
5	D5	35.5°C	71.9°C																																																																																																																																																					
6	D6	45.3°C	83.1°C																																																																																																																																																					
7	C6	33.0°C	68.5°C																																																																																																																																																					
8	D981	40.0°C	76.3°C																																																																																																																																																					
9	RY1	36.3°C	73.0°C																																																																																																																																																					
10	RG2	45.3°C	82.2°C																																																																																																																																																					
11	D431	46.3°C	81.4°C																																																																																																																																																					
12	C406	26.6°C	62.7°C																																																																																																																																																					
13	TSW4	34.2°C	70.6°C																																																																																																																																																					
14	L1	47.5°C	82.2°C																																																																																																																																																					
15	T951	39.7°C	75.8°C																																																																																																																																																					
16	C2	33.0°C	69.6°C																																																																																																																																																					
17	LF3	36.5°C	73.5°C																																																																																																																																																					
18	T1-1	51.5°C	87.4°C																																																																																																																																																					
19	T1-2	48.4°C	84.4°C																																																																																																																																																					
20	T2-1	49.9°C	85.6°C																																																																																																																																																					
21	T2-2	42.7°C	79.1°C																																																																																																																																																					
22	L900	43.3°C	80.2°C																																																																																																																																																					
23	Q910	50.1°C	90.1°C																																																																																																																																																					
24	C933	31.2°C	67.4°C																																																																																																																																																					
25	Q911	47.4°C	87.0°C																																																																																																																																																					
26	U900	30.4°C	66.6°C																																																																																																																																																					
27	C906	26.7°C	62.9°C																																																																																																																																																					
28	C106	30.9°C	67.2°C																																																																																																																																																					
29	C109	28.0°C	64.0°C																																																																																																																																																					
30	U501	33.0°C	69.7°C																																																																																																																																																					
31	Q502	44.3°C	81.2°C																																																																																																																																																					
32	Q504	43.1°C	79.6°C																																																																																																																																																					
33	U504	37.2°C	73.8°C																																																																																																																																																					
34	Q506	51.5°C	88.7°C																																																																																																																																																					
35	Q508	43.4°C	80.3°C																																																																																																																																																					
36	TSW3	27.6°C	63.7°C																																																																																																																																																					



2	OVER LOAD BURN-IN TEST	NO DAMAGE 1 HOUR (MIN)	I/P : 230 VAC O/P : 115 % LOAD Ta : 25°C	TEST : OK
3	LOW TEMPERATURE TURN ON TEST	TURN ON AFTER 2 HOUR	I/P : 230VAC/90VAC O/P : 100% /80% LOAD Ta= -45°C	TEST : OK
4	HIGH HUMIDITY HIGH TEMPERATURE HIGH VOLTAGE TURN ON TEST	AFTER 12 HOURS IN CHAMBER ON CONTROL 60 °C HUMIDITY= 90 %R.H NO DAMAGE	I/P : 272 VAC O/P : FULL LOAD Ta= 60°C HUMIDITY= 95 %R.H	TEST : OK
5	TEMPERATURE COEFFICIENT	± 0.03 %/°C (0-60°C)	I/P : 230 VAC O/P : FULL LOAD	± 0.009 %/°C (0-60°C)
6	STORAGE TEMPERATURE TEST	-40-85°C	1. Thermal shock Temperature : -45°C~ +90°C 2. Temperature change rate : 25°C / MIN 3. Dwell time low and high temperature : 30 MIN/EACH 4. Total test cycle : 10 CYCLE 5. Input/Output condition : STATIC	
7	THERMAL SHOCK TEST	-40-60°C	1. Thermal shock Temperature : -45°C~ +65°C 2. Temperature change rate : 25°C / MIN 3. Dwell time low and high temperature : 30 MIN/EACH 4. Total test cycle : 16 CYCLE 5. Input/Output condition : 15cycle:230V/ FULL LOAD AC ON 3sec/AC OFF 1sec TEST 1cycle:230V/ FULL LOAD Burn In Test	
8	VIBRATION TEST	10 - 500Hz, 5G 10min./1cycle, 60min. each along X, Y, Z axes	1 Carton & 1 Set (1) Waveform : Sine Wave (2) Frequency : 10-500Hz (3) Sweep Time : 12min/sweep cycle (4) Acceleration : 6G (5) Test Time : 180min in each axis (X.Y.Z) (6) Ta : 25°C	
9	CAPACITOR LIFE CYCLE	SUPPOSE C105 IS THE MOST CRITICAL COMPONENT (1) I/P : 230VAC O/P : FULL LOAD Ta= 25°C LIFE TIME (2) I/P : 230VAC O/P : FULL LOAD Ta= 60°C LIFE TIME (3) I/P : 230VAC O/P : 75% LOAD Ta= 60°C LIFE TIME (4) I/P : 230VAC O/P : 50% LOAD Ta= 60°C LIFE TIME		(1) 2272135HRS (2) 183566HRS (3) 236909HRS (4) 268024HRS
10	MTBF	Conducted by Parts Stress Analysis Prediction 286.3K hrs min. Telcordia SR-332 (Bellcore) ; 105.7K hrs min. MIL-HDBK-217F (25°C)		
11	DMTBF/Accelerated Life Test	Demonstration Mean Time Between Failure (Expected Life): Above 50,000 hours @ TA 60°C		

TEST RESULT	TESTER	REVIEW	APPROVAL
PASS	DANIEL GAO	SANFORD SU	VINCENT TSENG

12.10.30 A50-F031